



You may get one or more of the above **ERRORS** while opening your existing workbooks after EtaTrader/KiteNet update.


To rectify this error, you have to RE-COMPILE your each workbook once per computer or server.

(Close the Excel/Workbook WITHOUT saving if opened. Backup the workbook)

## 1. OPEN YOUR WORKBOOK IN SAFE MODE

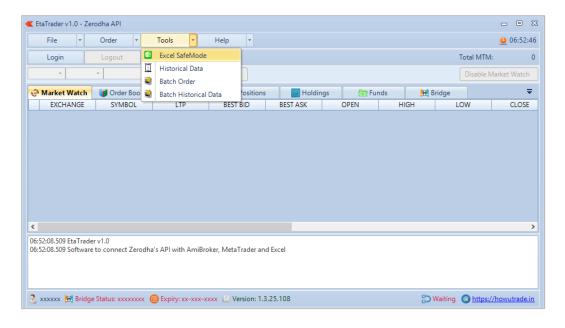

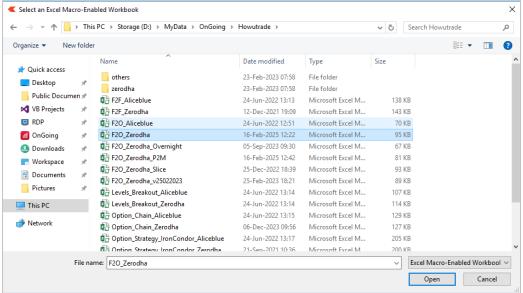

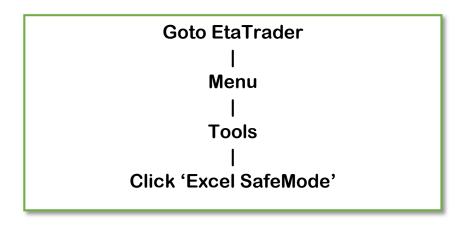


Select the required 'Excel Workbook'

Click 'Open'


(This will open the excel workbook in Safe Mode i.e. Macros Disabled)

# 2. OPEN VBA EDITOR AND EDIT CODE

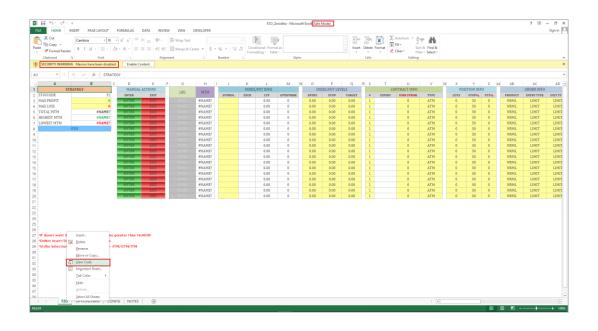

Right Click on ANY Sheet Name And Click 'View Code'


(This will open Excel VBA Editor)

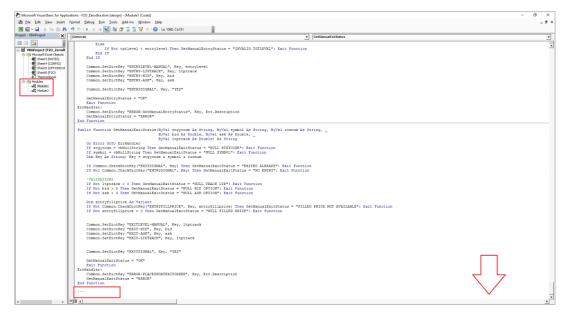

In the 'Project Explorer' (Left Side)
Expand the 'Modules' tree
Double Click on ANY Module


Goto the bottom of the VBA Code
Type " (Three Single Quote) and Press Enter

## 3. SAVE AND RE-COMPILE

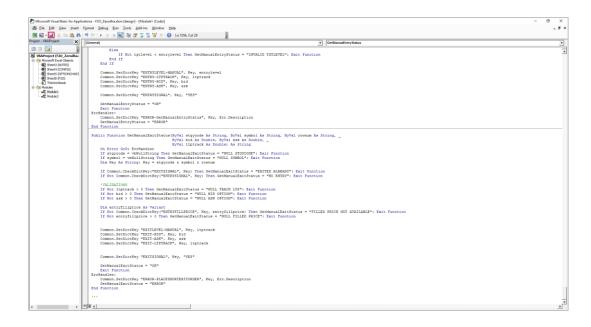


Extraction to the physications (15) Zeen Standard (1500) (15

Save the VBA Code by Clicking on the 'Save' icon

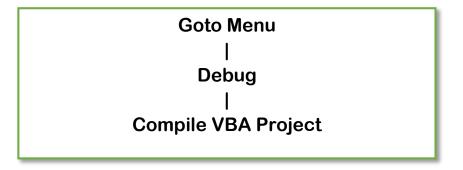


## 4. CLOSE VBA EDITOR

#### 5. SAVE AND CLOSE WORKBOOK

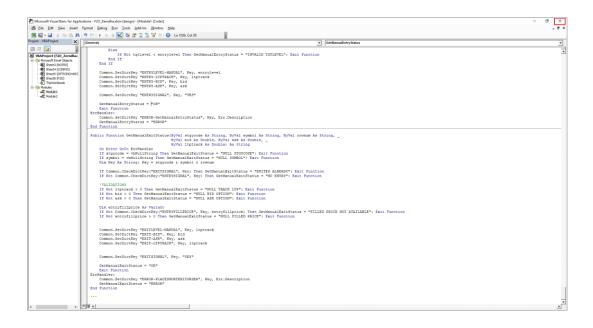

Close the VBA Editor

By Click on the Close Button

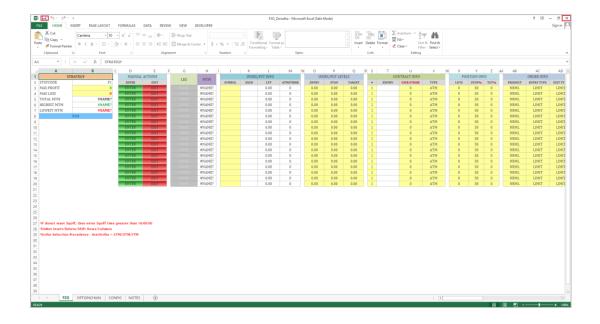

Save the Workbook by Clicking on the Save Icon

Close the Workbook

By Click on the Close Button

Now, you can open this workbook normally.

If the recompile is success then it won't throw any error.

(Same way recompile all the workbook once)